

## 产品分析证书 Certificate of Analysis

中文名称: 人参皂苷CK

English Name: Ginsenoside CK

别名 (Alias): Ginsenoside C-K

产品编码 (Cat. No.): BP0651


CAS Number: 39262-14-1

分子式 (M. F.): C<sub>36</sub>H<sub>62</sub>O<sub>8</sub>

分子量 (M. W.): 622.884

批号 (Batch No.): PRF8041906

报告日期 (Report date): 2017-04-20

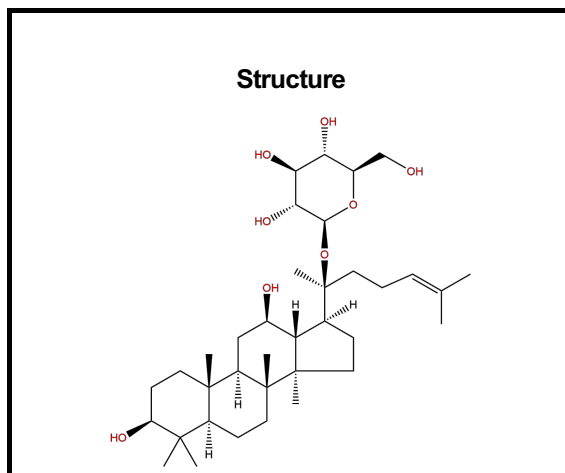

**检验结果 (Analytical result):**

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
纯度 Purity (HPLC-ELSD)*	≥98.0%	99.79%
质谱 Mass	622.8±1	Conforms
核磁 NMR	Comply with the structure	Conforms
水分 Water Content	<3.0%	2.2%

\* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo BDS Hypersil C18, 4.6\*100mm, 2.4um; Column temperature: 30°C; Detection Mode:

ELSD; Flow Rate: 0.8ml/min; Sample dissolution: Methanol; Mobile Phase: A, Water B, Acetonitrile; Gradient elution: B, 45%-65%, 15min.

贮存条件 (Storage): -2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-04-19) under conditions list above.

QC: Zhang Ling

Date: 2017-04-20

QA: Wu Qi

Date: 2017-04-20

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.




Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

**SAMPLE INFORMATION**

Sample Name:	Ginsenoside CK PRF8041906	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	3	Acq. Method Set:	Ginsenoside CK
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	SATIN
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	
Date Acquired:	2017-4-20 9:09:14 CST		
Date Processed:	2017-4-20 9:43:51 CST		

**Auto-Scaled Chromatogram**

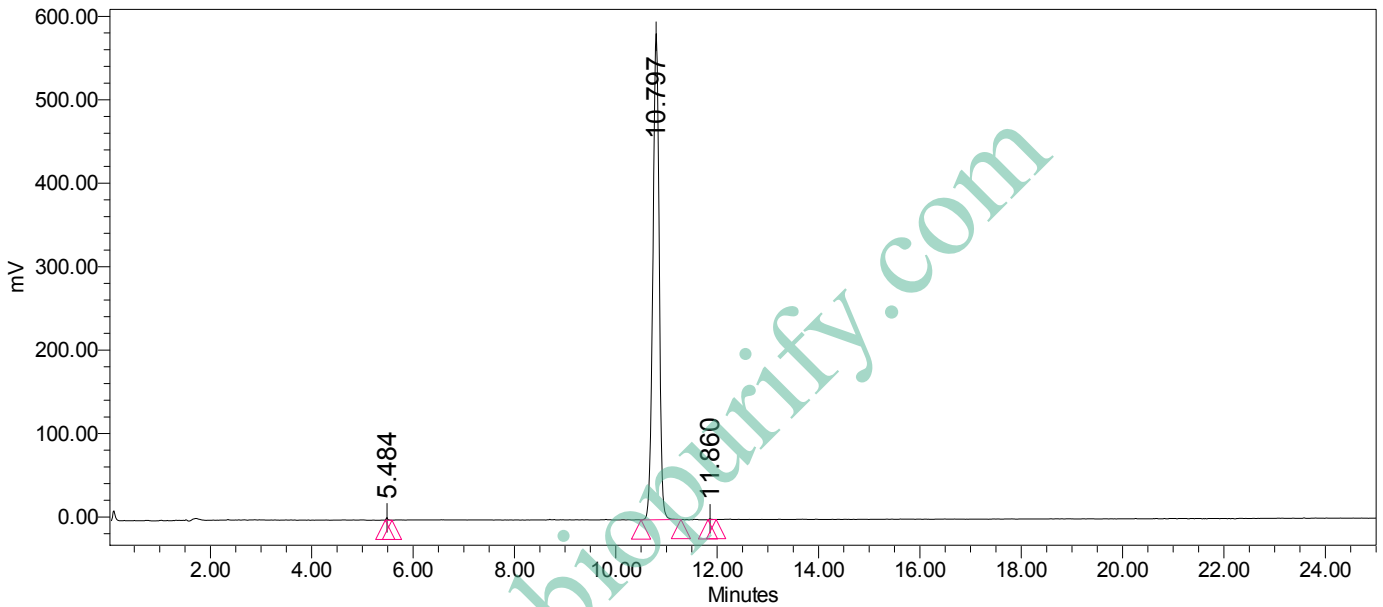

**Peak Results**

Name	RT	Area	% Area	USP Plate Count	USP Resolution
1	5.484	7459	0.15	104399.0	
2	10.797	5026465	99.79	35808.6	35.9
3	11.860	3262	0.06	477652.0	6.8